


Product Datasheet

Neutral Xylanase Microplate Assay Kit (orb390795)

Description	Detection and Quantification of Neutral Xylanase Activity.
Reactivity	All
Range	0.01 mmol/L - 1 mmol/L
Tested Applications	FA
Storage	Shipped and store at 4°C for 6 months.
Note	For research use only
Application notes	Detection Method: Colorimetric Sample Types: Animal feeds, Enzyme preparations, Bread improver mixtures and other materials
Sample Types	Animal feeds, Enzyme preparations, Bread improver mixtures, other materials
CAS Number	9025-57-4
Expiration Date	12 months from date of receipt.

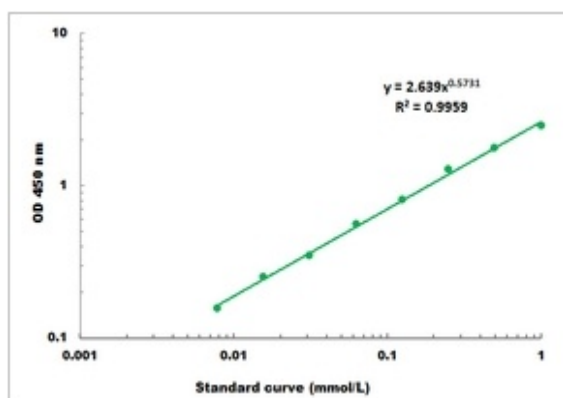


Representative Standard Curve

Biorbyt Ltd.

7 Signet Court, Swann's Road,
Cambridge, CB5 8LA, United Kingdom
Email: info@biorbyt.com, support@biorbyt.com
Phone: [+44 \(0\) 1223 859-353](tel:+44(0)1223859353) | Fax: [+1 \(415\) 651-8558](tel:+1(415)6518558)

Biorbyt LLC.

68 TW Alexander Drive,
Durham, NC, 27713, United States
Email: info@biorbyt.com, support@biorbyt.com
Phone: [+1 \(415\) 906-5211](tel:+1(415)9065211) | Fax: [+1 \(415\) 651-8558](tel:+1(415)6518558)

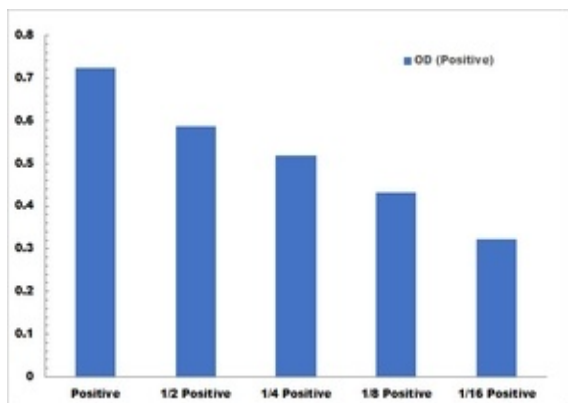

Positive Control reaction in 96-well plate assay with decreasing the concentration

Biorbyt Ltd.

7 Signet Court, Swann's Road,
Cambridge, CB5 8LA, United Kingdom
Email: info@biorbyt.com, support@biorbyt.com
Phone: [+44 \(0\) 1223 859-353](tel:+44(0)1223859353) | Fax: [+1 \(415\) 651-8558](tel:+1(415)6518558)

Biorbyt LLC.

68 TW Alexander Drive,
Durham, NC, 27713, United States
Email: info@biorbyt.com, support@biorbyt.com
Phone: [+1 \(415\) 906-5211](tel:+1(415)9065211) | Fax: [+1 \(415\) 651-8558](tel:+1(415)6518558)